


PRV

PATENT- OCH REGISTRERINGSVERKET
Patentavdelningen

PCT / SE 2005 / 000203

Intyg Certificate

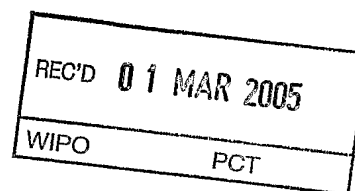

Härmed intygas att bifogade kopior överensstämmer med de handlingar som ursprungligen ingivits till Patent- och registreringsverket i nedannämnda ansökan.

This is to certify that the annexed is a true copy of the documents as originally filed with the Patent- and Registration Office in connection with the following patent application.




(71) Sökande Karl Andersson, Uppsala SE
Applicant (s)

(21) Patentansökningsnummer 0400403-2
Patent application number

(86) Ingivningsdatum 2004-02-20
Date of filing

Stockholm, 2005-02-18

För Patent- och registreringsverket
For the Patent- and Registration Office

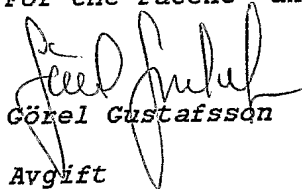
Görel Gustafsson

Avgift
Fee

PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

PATENT- OCH
REGISTRERINGSVERKET
SWEDEN

Postadress/Adress
Box 5055
S-102 42 STOCKHOLM

Telefon/Phone
+46 8 782 25 00
Vx 08-782 25 00

Telex
17978
PATOREG S

Telefax
+46 8 666 02 86
08-666 02 86

METHOD AND DEVICE FOR THE CHARACTERIZATION OF INTERACTIONS BETWEEN DIFFERENT SPECIES

FIELD OF INVENTION

5 The present invention relates to the field of characterization of how different species interact with each other. More in particular, it relates to a method where one or more of the species are attached to a solid support and the other species are put in a liquid that is contacting the solid support. Even more in particular, it relates to the interaction of species of biological or
10 chemical origin, e.g. cells, proteins, DNA, RNA, tissue, synthesized chemical compounds and the like.

BACKGROUND OF THE INVENTION

Interactions between different species are important in living organism and
15 in industrial systems. The immune system is a first example, where antibodies in the bloodstream interact with pathogens and thereby guide natural killer cells to the pathogen. Therapeutic drugs is a second example, where a drug may interact with an enzyme in a way that inhibit the enzyme activity. A third example is detection of diseases in humans or animal, by
20 contacting a sample from the human or animal with a liquid containing a species that interacts specifically with the pathogen causing the disease. If the species remains on the sample after a wash step, the sample is carrying the pathogen causing the disease. Exactly the same method can be used to detect contamination in food stuff. This means that methods and devices for
25 characterization of interactions between species are important not only for research and diagnostics in biology and medicine, but also in quality control and characterization assays in a variety of fields.

There are many known methods for characterizing the interaction between
30 two or more species. One common method is to attach one species to a solid support and add a second bifunctional species dissolved in liquid. The bifunctional species should (a) have a property that is easily detectable (e.g.

be radioactive or have a fluorescent moiety attached to it) and (b) interact with the species that is attached to the solid support. The liquid is brought into contact with the solid support, sometimes followed by a wash of the solid support in a liquid without the bifunctional species. If the bifunctional species interacts stably with the species on the solid support it will
5 accumulate on the solid support and remain there after a wash. Presence of the bifunctional species can then be detected. Another, more complicated method that has been widely used for the characterization of interactions is enzyme linked immunosorbent assay (ELISA).

10

The present invention aims at facilitating the characterization of how species interact with each other. The method is particularly suitable when one of the species is large (in a molecular context), e.g. if one of the species is cells or bacteria.

15

CLOSEST PRIOR ART

Pierce Biotechnology Inc (Rockford, IL, United States of America) manufactures and sells a microplate where the bottom of each well has up to 16 defined areas where antibodies that recognize specific proteins are
20 attached (Searchlight™). When a liquid sample is put in a well the specific proteins are bound to the different areas on the bottom of the well. The detection of the different proteins is mediated by secondary antibodies, one for each specific protein, labeled with a moiety that emits light. A camera is then used to quantify the light intensity, which is related to the specific
25 protein concentration, on each defined area. This method is presently limited to proteins and does not explicitly use one defined area for reference purposes. A detailed description of the Searchlight™ method may be found in an article by MD Moody, SW Van Arsdell, KP Murphy, SF Orencole and C Burns (Biotechniques (31(1):186-90, 192-4, Jul 2001) which is incorporated
30 by reference herein.

Biacore AB (Uppsala, Sweden) manufactures an optical biosensor (Biacore®3000) that has a solid support with 4 defined areas where different species can be attached. Liquid samples are injected onto the solid support. If a species present in the liquid is binding to the species attached to the solid support, the refractive index close to the solid support will change. The optical detection system monitors refractive index close to the solid support in real time. When operating this instrument, it is recommended to use one of the defined areas for reference purposes. The liquid that is in contact with the solid support is however not stirred, instead there is a continuous flow of liquid over the solid support. Although the Biacore®3000 was primarily designed to monitor interactions between proteins, interactions between cells and proteins have been monitored. A detailed discussion of the technical aspects of the BIACORE instrument may be found in U.S. Patent No. 5,313,264 which is incorporated by reference herein.

SUMMARY OF THE INVENTION

The object of the present invention is to facilitate the characterization of how different species interact with each other. In a first aspect the invention provides a method for the characterization of interaction between species. This method is defined in claim 1.

In a further aspect, the invention provides a device for carrying out the method. The device according to the invention is defined in claim 10.

The invention in a preferred embodiment has four characteristic features.

- A solid support with at least two defined areas, namely one for a target and at least one for reference purposes. However, several different targets can be provided in separate areas. A liquid containing a ligand is in contact with the solid support to enable an interaction between target and ligand.

Pat. No. 018 568939

Pat. No. 018 568939

Pat. No. 018 568939

4

- A detector is arranged so as to be able to detect and quantify the presence of the ligand on the defined areas.
- Preferably stirring of the liquid in contact with the solid support is provided for.
- 5 • An essential feature is provision of means for at least temporarily reducing the amount of solution at a defined area during detection.

By quantifying the amount of ligand on all defined areas it is possible to use the reading from the reference area as a background signal. The detected
10 amount of ligand bound to the species that is attached to the solid support can then be corrected for the background signal. There are two reasons for stirring the liquid. Firstly, the liquid will be homogenous in the container and secondly, the time required to reach equilibrium will not be increased due to slow diffusion of the ligand in the liquid.

15

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention will be disclosed in closer detail in the description and example below, with reference to the accompanying drawing, in which

20

Figure 1 shows a schematic of one possible instrument design;
Figure 2a shows data acquired with a very low concentration of the ligand;
Figure 2b shows data acquired with a high concentration of the ligand;
Figure 3a and 3b illustrates how the acquired data is processed prior to
25 evaluation; and
Figure 4 shows how different concentrations of a ligand give rise to different signals.

25

DETAILED DESCRIPTION OF THE INVENTION

30

For the purpose of the present application, and for clarity, a species that is attached to the solid support is denoted "target" and a species present in a

liquid is denoted "ligand". Possible species (i.e. targets and ligands) include, but are not limited to, tissue samples, cells, bacteria, viruses, solid particles, macromolecules (e.g. proteins, DNA, RNA) and other chemical compounds.

- 5 The present invention aims at improving the accuracy and precision of the characterization of interactions between different species. And reducing the labor time required for performing a characterization.

- 10 Generally, a device for detecting interactions between species in solution and species on a solid support according to the invention, comprises: a solid support (11) on which a first species can be attached; a mechanism (16) adapted for temporarily reducing the amount of a solution to which said support is exposed in the course of a measurement, in a selected area of said support; a detector (12) capable of detecting an interaction between
15 said first species attached to the solid support, and a second species contained in said solution, in said selected area.

- 20 Preferably the solid support is an essentially flat dish capable of holding a solution confined within its boundaries, such as a Petri dish, although any other kind of receptacle or vessel capable of confining solution is possible.

- The device is suitably provided a motor for enabling rotation of the dish at an angle deviating from the horizontal, so as to provide for a reduction of the amount of solution in said selected area of said support.

- 25 In order to remove solution, the invention provides in one embodiment an aspirating device for aspirating solution from said support before measurement, and for returning solution to the support after measurement.

- 30 Preferably, the detector (12) is a scintillation detector, although many other types of detectors are possible, see below.

The method according to the invention, which is suitably carried out with a device such as the one described, comprises attaching a first species (target) on a selected portion of a solid support. Then, said first species is exposed to a solution containing a second species, commonly referred to as a target. A measurement, capable of detecting an interaction between said first and said second species is performed. According to the invention, the amount of solution covering the selected portion of the support, where the first species is attached, is reduced prior to performing said measurement. Suitably, a reference measurement is performed on a portion of said support where no interaction takes place, suitably where no target is attached.

The sequence of steps of exposing, measuring and reducing the amount of solution is preferably repeated, and the concentration of said second species is increased by a finite amount before said sequence of steps is repeated.

In a preferred embodiment of the method, the reduction of the amount of solution is achieved by orienting the support at an angle that deviates from the horizontal to provide an elevated part and a lower part of said support, such that the elevated part will be covered by less solution than the lower part, and wherein the support is rotated at a predetermined speed of rotation.

According to one embodiment of the invention, a device comprising four main characteristics is used for the characterization of interactions between ligands and targets. Namely, on one single solid support two or more areas are defined, where at least one area is reserved for attaching a target (also referred to as an active area) and at least one area is reserved for reference purposes. A reference area either has nothing attached to it or has an irrelevant target attached to it. Furthermore, liquid containing a ligand is in contact with the solid support. There is also a detection system able to detect presence and quantity of the ligand on each area. There is a mechanism for stirring the liquid present on the solid support. Finally, there

is a mechanism that ensures that the amount of liquid present close to a defined area is temporarily reduced during detection.

5 Since the same liquid contacts the active area (target) and the reference area and separate detection of presence of ligand on the active and reference areas, respectively, is possible, a background correction is obtained by subtracting the detector output for the reference area from the active area. Also, since the liquid is stirred, the time required to reach equilibrium will decrease compared to when the solid support and liquid is left still.

10

Commonly used methods for characterization of interactions between targets and ligands often include a wash step. The purpose is to remove all ligand that has not bound to the target, since presence of unbound ligand may be detected. Advantageously, in the present invention, a wash step is
15 not necessary due to the use of a reference area. However, a wash step can increase the sensitivity at high concentrations of ligand present in the liquid.

20

Since a wash step is not required, solution containing ligand can be reused throughout a characterization. This is of particular interest when the ligand is expensive. In this case, a liquid with low concentration of ligand is put into contact with the solid support. After characterization of this first concentration a small aliquot of highly concentrated ligand is added. The total concentration of ligand then increases to a second level, and the
25 binding is characterized. This process is repeated until the desired concentrations have been characterized.

30

The solid support is typically a container. In this container two or more defined areas are present. Liquid put in the container contacts all defined areas. At least one defined area is always reserved for reference purposes. This makes it possible to characterize the interaction of one ligand with several targets simultaneously. Another possibility is the use a detection

system that can distinguish different ligands, e.g. by attaching different fluorescence dyes on the different ligands and detecting the light intensity at the different characteristic emission wavelengths corresponding to the selected dyes. With this setup, several ligands can be put in one liquid and
5 binding of all ligands to one or more targets can be characterized simultaneously.

The attachment of target on the defined areas can be performed in a variety of ways. Cells could be grown directly on a defined area. The defined areas
10 could be coated with a protein known to enhance attachment of cells. The defined areas could be coated with a protein known to bind a specific molecule which is used for attachment of the target. One such protein is streptavidin which binds biotin strongly. A biotinylated target (e.g. biotinylated DNA) could then be conveniently attached as target to the
15 defined area. The surface of the defined areas could be chemically modified to make possible covalent attachment of a target. Passive adsorption of target directly onto the defined area is also possible. The surface of the defined areas is not necessarily solid and flat. Porous surfaces or surfaces with biopolymers attached (e.g. polyethylene glycol or dextran) could be
20 advantageous due to increased target density making a higher signal possible.

The defined areas on the solid support do not need to be explicitly marked. When growing cells are used as target, a drop of cells can be put on the solid
25 support, leaving the majority of the solid support clean for reference purposes. When the cells have sedimented and started to attach to the solid support more liquid (without cells) can be carefully added to the solid support to prevent the cells from drying. It is also possible to physically divide the solid support into defined areas by use of low ridges or the like.
30 The ridges should be high enough to prevent liquid from reaching other defined areas during attachment of target, but low enough to let liquid contact all defined areas simultaneously during measurement.

This method can use several different detection principles. Two different types of detector set-ups are possible: Detectors that are in physical contact with the solid support and detectors that are not in physical contact with the solid support. Detector principles that do require physical contact with the solid support include (but are not limited to) electrochemical detection of ligand, refractometric detection of ligand. Detector principles that do not require physical contact with the solid support include (but are not limited to) detection of radioactivity, detection of emitted light (e.g. using fluorescence or chemoluminescence), spectrophotometric detection, just to mention a few. The detection system used in this method is time resolved. This means that detection of a defined area is repeated at least every tenth minute, preferably every 30-60 seconds, even more preferably every 1-10 seconds. The time-resolved measurement makes it possible to monitor the rate of ligand binding to the target, also known as the kinetics of the interaction.

A mechanism that temporarily decreases the amount of liquid in the vicinity of the defined area during detection is beneficial but not necessary. The method relies on differential measurements (i.e. signal from active area minus signal from reference area) and as such it should not, in theory, be affected by excess of liquid present in the vicinity of the defined area during detection. In practice, performance may increase when such excess liquid is temporarily removed. The problem is that for some detection principles, e.g. detection of radioactivity, the amount of ligand present in a volume close to the detector will be detected. This volume includes the active area and the liquid present on the active area. The amount of unbound ligand present in the liquid will often be much larger than the amount of ligand bound to the target, which means that the detector will register almost the same amount of radioactivity during detection of an active area and a reference area. The resolution for such differential measurements can sometimes be low. This problem can be overcome by temporarily reducing the amount of solution

covering the solid support. One possible method is to use a circular solid support (e.g. a cell dish) and put defined areas along the perimeter of the solid support. If such a solid support is placed on a rotating disk that is mounted with a slight slope it becomes possible to position a selected

5 defined area at the highest position during detection. Liquid present on the solid support will accumulate in the lower end of the solid support and will not severely impact the quantification of ligand on the selected defined area. Another possible method for temporarily moving liquid on the solid support is to tilt the solid support during detection. If the defined areas are put in

10 one end of a solid support and this end is elevated during detection, liquid present on the solid support will accumulate in the other end and make a more reliable detection possible. A third possible method is to use a pump that aspirates the liquid on the solid support during detection, and dispenses the liquid back onto the solid support afterwards. It is notable

15 that all these methods also provide a stirring of the liquid present on the solid support. The amount of liquid that remains on the defined area during detection should be less than 10%, preferably less than 5% and even more preferable less than 1% of the amount of liquid present in the vicinity of the defined area when the solid support is positioned horizontally in rest. This

20 could be measured using a solid support without any target attached to the defined areas and compare the signal from a defined area in horizontal position with the signal from the same defined area in position for detection with the liquid temporarily removed.

25 If stirring is not obtained from the method of temporarily removing liquid from the solid support, a stirring device is required. This could be a vibrating rod or a rotating propeller that is put in the liquid. Alternatively, the solid support could be moved repeatedly to induce movements in the liquid. Possible motions include gentle shaking and excentric rotation.

30 In a further aspect of the invention, a solid support designed for use with the method according to the invention is provided.

11

The physical structure of one embodiment of a device according to the invention is illustrated in figure 1. For this embodiment a radioactively labeled ligand is used, whereby the target will become radioactive when
5 ligand binds thereto. The device comprises two key components.

- (i) a cell dish support that can be rotated slowly 11.
- (ii) a time-resolved scintillation counter 12 mounted such that it will detect interactions present only on a peripheral part of the cell dish.

10

A stepper motor 16 is connected to the cell dish support 11. The motor is controlled by an electronic device 14 that both can adjust the angular position and report the angular position of the cell dish support. The scintillation detector 12 is connected to an electronic device 13 that counts
15 the number of impulses from the detector 12. The cell dish support is inclined and the scintillation counter is located at the highest point of the cell dish support. The scintillation counter is read with a high frequency to allow multiple activity measurements during one round. A computer 15 synchronizes scintillation counter output from 13 and the angular position
20 of the cell dish support from 14 and generates an activity versus angular position curve.

The target, here human cancer cells, are grown only on a limited sector of the cell dish, as indicated in white in figure 1. A liquid containing the ligand,
25 in this case a radioactively labeled protein, is added to the cell dish. It is known that the ligand binds to receptors present on the target cell surface. As the dish rotates, the activity of the dish bottom will be continuously monitored, sometimes an area with target cells, sometimes an area without target cells. If the ligand binds to the target cells, an increase of the
30 radioactivity will be registered by the scintillation counter when the target cell sector of the cell dish passes the detector.

The four (main) features of the invention mentioned previously can be embodied as described below.

- The solid support, i.e. the cell dish, has a limited area with target cells on.
- 5 The remaining area of the cell dish is used for reference purposes. The detector is mounted in a peripheral part of the cell dish. When the cell dish rotates, the radioactivity is frequently registered. This makes it possible to plot degree of radioactivity (i.e. the amount of ligand) versus position on cell dish perimeter. The stirring is obtained by mounting the cell dish non-
- 10 horizontally. When the cell dish rotates, the liquid will start to rotate but with a different speed than the cell dish. The temporary removal of liquid is also obtained by mounting the cell dish non-horizontally. The detector is mounted near the highest point of the cell dish which is the point where there is the least amount of liquid.

- 15 The following non-limiting example of the invention will illustrate the principle behind it.

EXAMPLE

- 20 The instrument described above was tested with U343 cells grown on one quarter of a 10cm circular cell-dish. The dish was rotated with a speed of approximately 6 rounds per minute. It is important to select a proper rotational speed for the dish. If the dish rotates too fast the liquid present in
- 25 the dish will not have time to accumulate in the lower end of the dish yielding a poor temporary removal of liquid near the detector. If the rotation is too slow the measurements of the active area and the reference are too distant in time to justify a differential measurement. Rotational speeds proper for the instrument in this example range from approximately 1 round
- 30 per minute to approximately 1 round per second. 2ml of liquid containing increasing concentrations of EGF (Epidermal Growth Factor) labeled with ¹²⁵I was added to the cell-dish. EGF is known to bind to the EGF receptor,

13

and U343 cells are known to have high levels of EGF receptors on their surface. The radioactivity was measured at least 2 times per second giving approximately 20 measurements per round. Since EGF is known to bind to the cells, the measured radioactivity will be higher when the area of the cell-dish holding target cells passes by the detector compared to other times.

5 This gives a continuous wave-like time series where the period is determined by the angular speed of the dish and the amplitude by the amount of EGF binding to the cells.

10 In figure 2, two time-series are plotted, one with a low concentration of EGF and one with a higher concentration. The y-axes in figure 2 have the unit counts per second (cps), i.e. the number of ^{125}I decays per second. At the low concentration, there is no obvious pattern in the time series. This means that the amount of EGF bound to the target cells was very low. At the higher

15 concentration, a clear wave-like pattern appears, proving that EGF is bound specifically to the part of the cell-dish where there actually are cells. In order to increase the precision a 3-6 minute long time-series was obtained for each concentration EGF. All peaks in the time-series were then identified, peak-to-peak fragments were cut, overlayed and averaged as outlined in

20 figure 3. The amplitude of the thicker average line was used as signal for the measurement, as illustrated by the arrow.

In order to collect a binding curve for radiolabeled EGF binding to U343 cells, 8 different concentrations of radiolabeled EGF were added to one cell

25 dish put in the instrument [experiment 020905a]. The sequence of operation was:

1. Add 4ml of medium + radiolabeled EGF. Rotate dish for 500s.
2. Take a 200ul aliquot of the medium + radiolabeled EGF liquid to
- 30 make concentration determination possible.
3. Wash the cell dish with 4-8ml medium (this step was omitted for the three lowest concentrations).

14

4. Add 4ml of medium. Record the radioactivity (time resolved) during 500s.
 5. Repeat step 1-4 with increasing concentrations of radiolabeled EGF.
- 5 The signal for each sample was determined as described above, by overlaying peak-to-peak fragments, averaging and extracting the wave amplitude. A signal versus concentration plot is found in figure 4. It clearly resembles the sigmoidal curve expected from a binding experiment. The first three samples were measured directly without a wash step (point 3 in the
- 10 sequence of operation above), which explains the discontinuity between sample 3 and sample 4.

- Although the invention has been described with regard to its preferred embodiment, which constitute the best mode currently known to the
- 15 inventor, it should be understood that various changes and modifications as would be obvious to one having ordinary skill in this art may be made without departing from the scope of the invention as set forth in the claims appended hereto.

CLAIMS:

1. A device for detecting interactions between species in solution and species on a solid support, comprising:
 - 5 a solid support (11) on which a first species can be attached;
 - a mechanism (16) adapted for temporarily reducing the amount of a solution to which said support is exposed in the course of a measurement, in a selected area of said support;
 - a detector (12) capable of detecting an interaction between said first
10 species attached to the solid support, and a second species contained in said solution, in said selected area.
2. Device as claimed in claim 1, wherein said solid support is an
15 essentially flat dish capable of holding a solution confined within its boundaries.
3. The device as claimed in claim 1 or 2, wherein there is provided a motor for enabling rotation of the dish at an angle deviating from the horizontal, so as to provide for a temporary reduction of the amount of
20 solution in said selected area of said support.
4. The device as claimed in claim 1 or 2, wherein there is provided an aspirating device for aspirating solution from said support before measurement, and for returning solution to the support after measurement.
25
5. The device as claimed in any of claims 1 - 4, wherein the detector (12) is a scintillation detector, and wherein there is further provided an electronic counter device (13) for counting the impulses from the detector (12), and a control unit for adjusting and reporting the angular position of
30 the support (11), and a computer (15) for synchronizing scintillation counter output from the counter (13) and the angular position of the cell dish support from the control unit (14).

6. A method of detecting interactions between species in solution and species on a solid support, comprising:

5 attaching a first species on a selected portion of a solid support;

exposing said first species to a solution containing a second species;

10 performing a measurement, capable of detecting an interaction between said first and said second species;

characterized in that

15 the amount of solution covering the selected portion of the support is reduced prior to performing said measurement;

a reference measurement is performed on a portion of said support where no interaction takes place.

20 7. The method as claimed in claim 6, wherein a difference between target and reference measurements is calculated.

25 8. The method as claimed in claim 6 or 7, wherein the sequence of steps of exposing, reducing the amount of solution, and measuring is repeated, and wherein the concentration of said second species is increased by a finite amount before said sequence of steps is repeated.

30 9. The method as claimed in any of claims 6-8, wherein the solid support is an essentially flat dish capable of holding a solution confined within its boundaries.

10. The method as claimed in any of claims 6-9, wherein the reduction of the amount of solution is achieved by orienting the support at an angle that deviates from the horizontal to provide an elevated part and a lower part of said support, such that the elevated part will be covered by less solution than the lower part, and wherein the support is rotated at a predetermined speed of rotation.

11. The method as claimed in any of claims 6-10, wherein the first species is selected from tissues, cells, bacteria, virus particles.

ABSTRACT

The invention relates to a device for detecting interactions between species in solution and species on a solid support. It comprises a solid support (11),
5 a mechanism (16) for temporarily reducing the amount of a solution to which said support is exposed, a detector (12) capable of detecting an interaction between species attached to the solid support, and species contained in said solution. The invention also relates to a method
10 comprising attaching a first species on a solid support, exposing said first species to a solution containing a second species, performing a measurement, capable of detecting an interaction between said first and said second species, and a reference measurement. The solution is temporarily removed during the measurement

15 (Fig. 1)



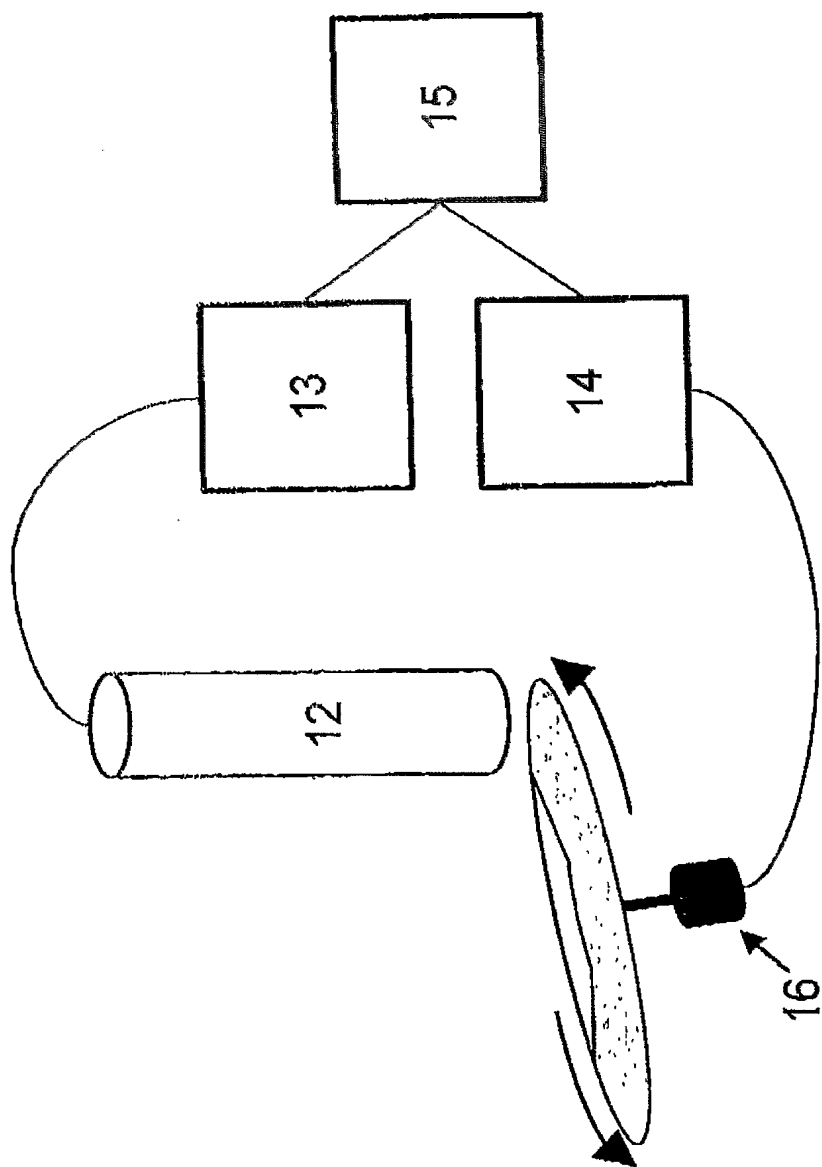


Figure 1

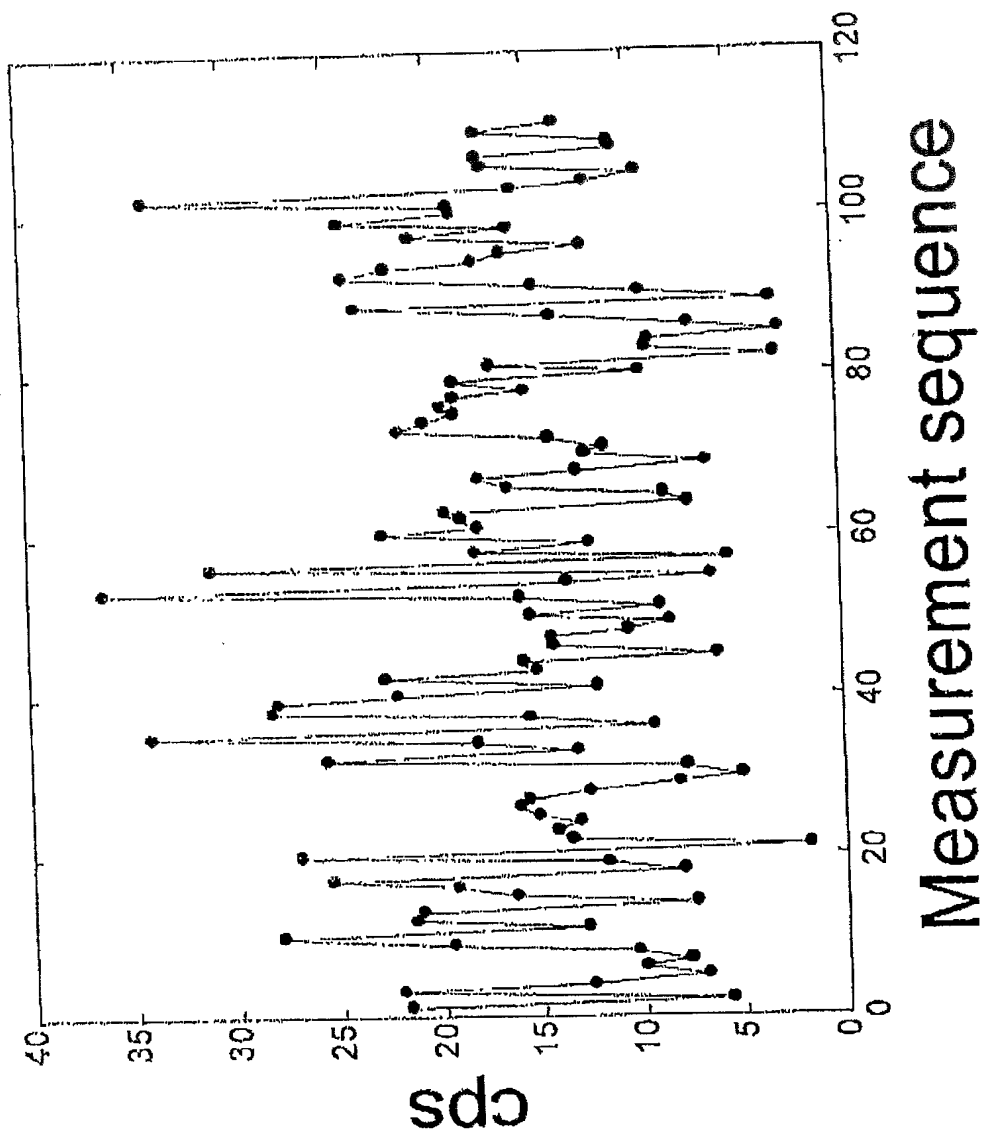


Figure 2a

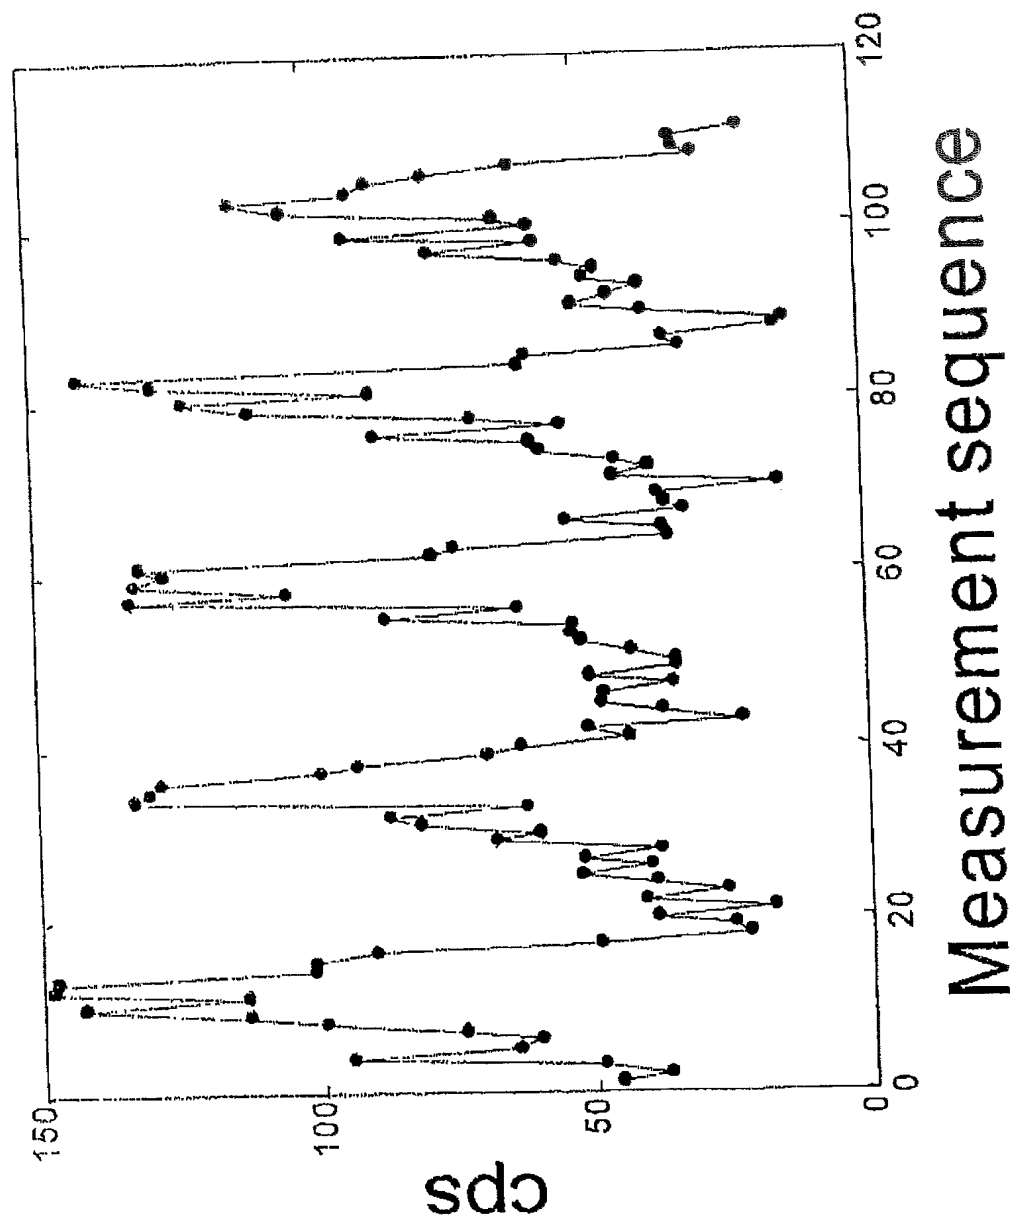


Figure 2b

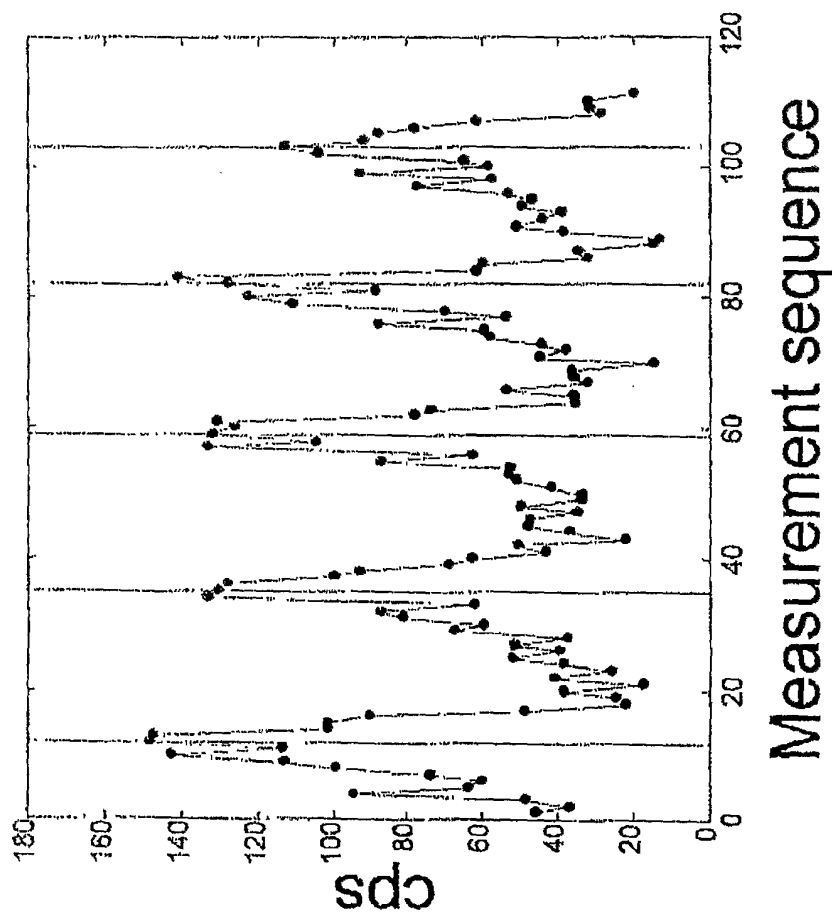


Figure 3a

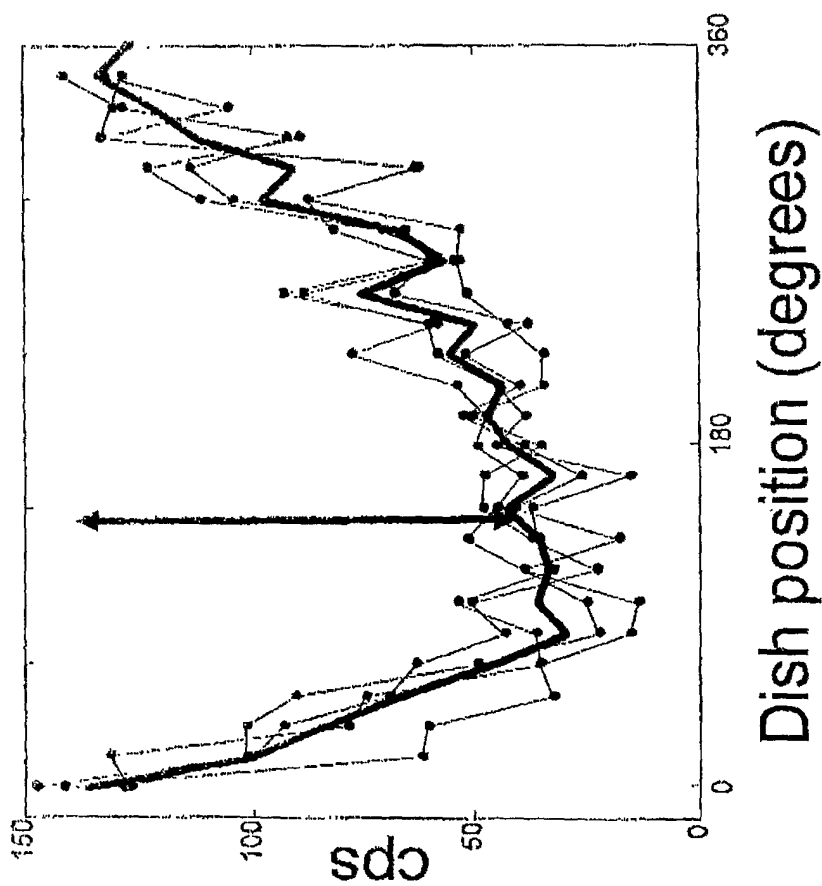


Figure 3b

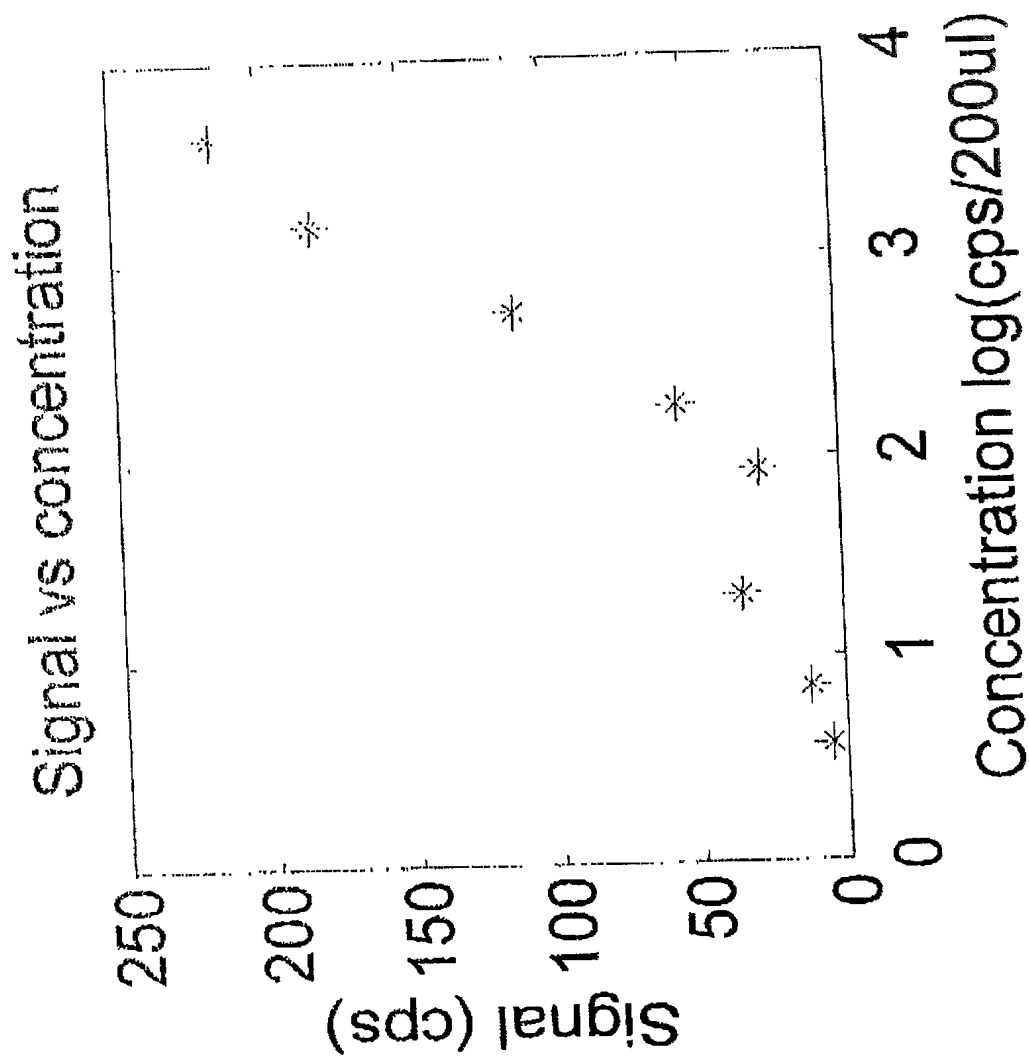


Figure 4